


## MED-125

### Installation dimensions

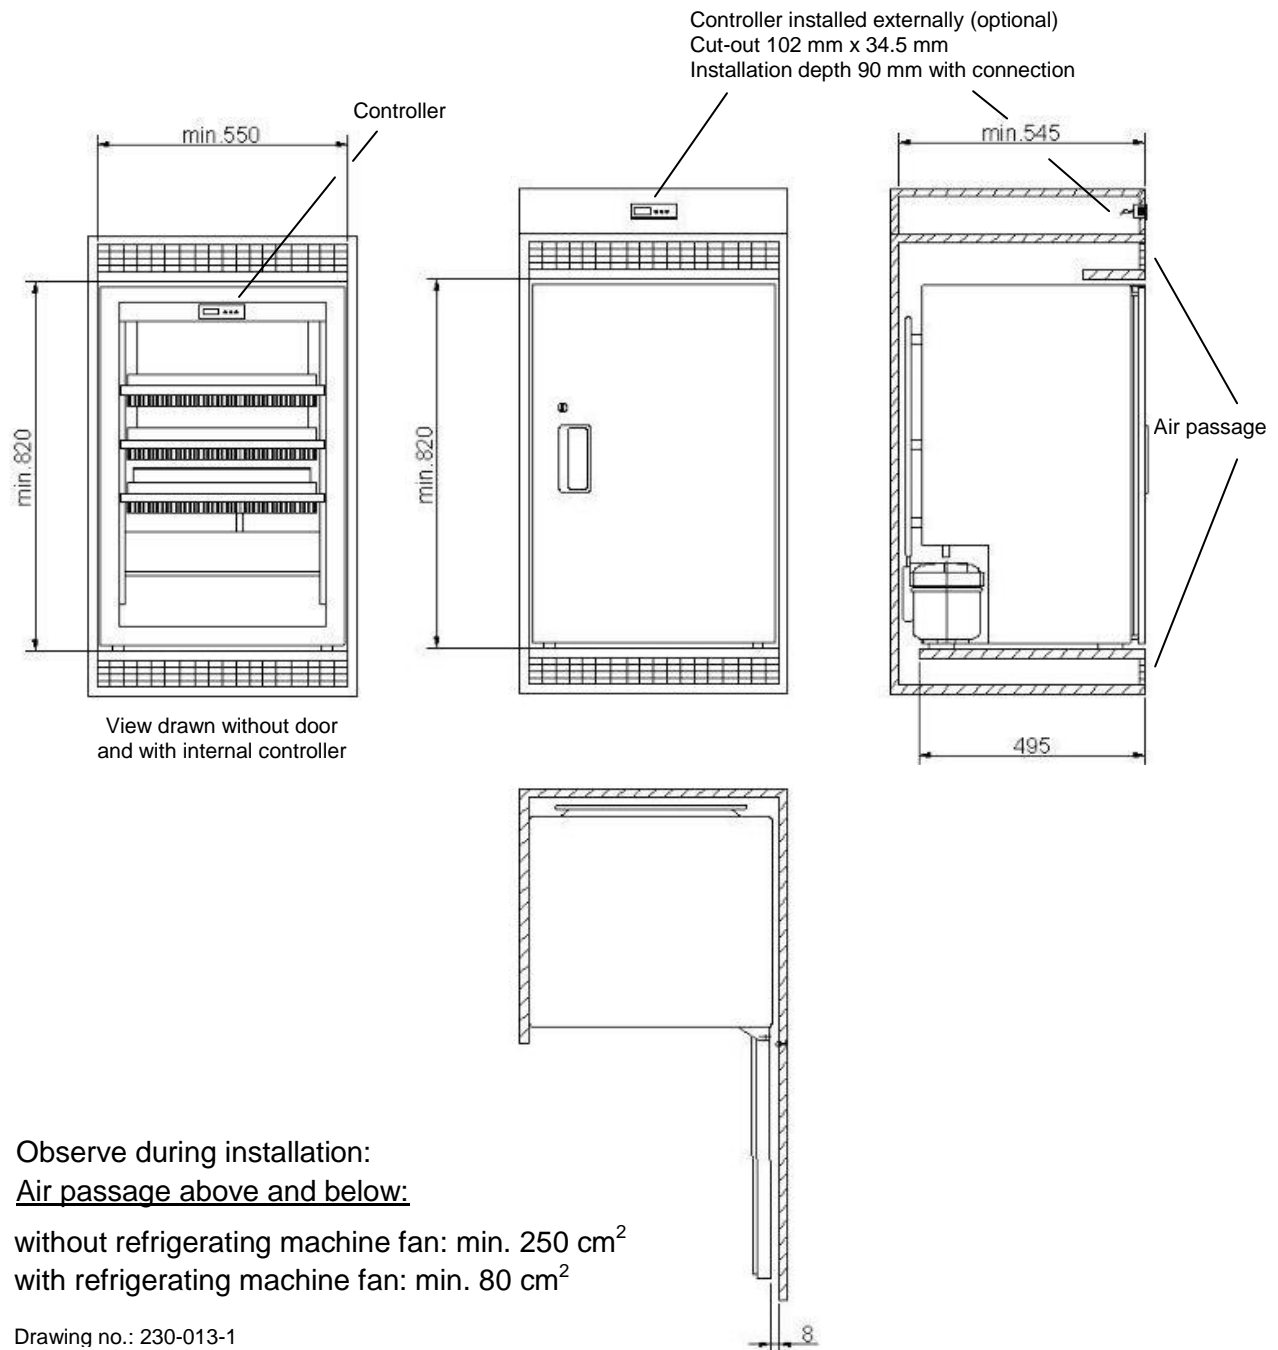

Observe during installation:

Air passage above and below:

without refrigerating machine fan: min. 250 cm<sup>2</sup>

with refrigerating machine fan: min. 80 cm<sup>2</sup>

Drawing no.: 230-013-1